





<u>G</u>.1

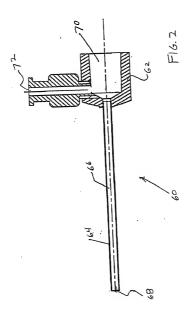


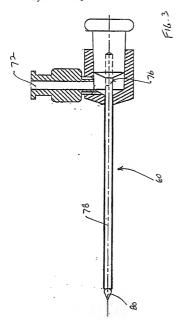



301499.3000-100 MINIATURE ENDOSCOPE WITH IMAGE FIBER SYSTEM By: Paul Remijan et al.

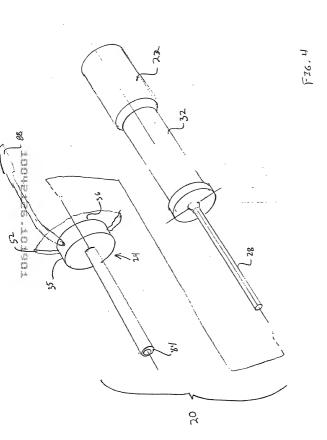

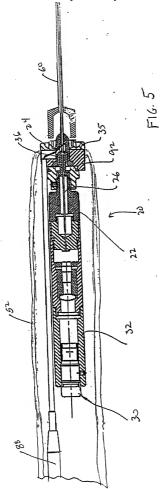

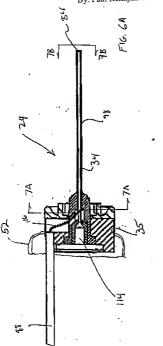





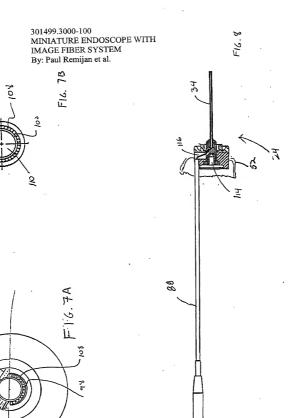


301499.3000-100 MINIATURE ENDOSCOPE WITH IMAGE FIBER SYSTEM By: Paul Remijan et al.








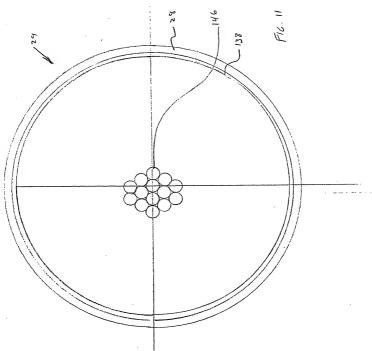



301499.3000-100 MINIATURE ENDOSCOPE WITH IMAGE FIBER SYSTEM By: Paul Remijan et al. -MAX SINE OF RAY ANGLE 70 DEG LENS F16. B RAY ANGLES VS IMAGE HEIGHT The Court of the C 9.0 NORMALIZED IMAGE HEIGHT


0.05


301499.3000-100 MINIATURE ENDOSCOPE WITH IMAGE FIBER SYSTEM By: Paul Remijan et al.

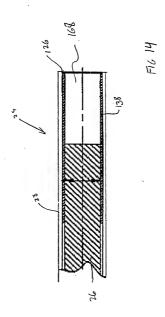


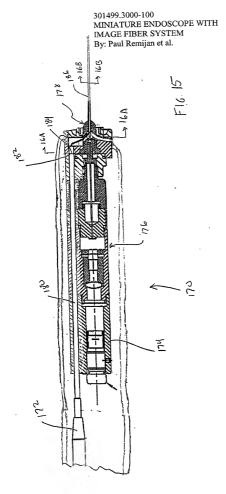

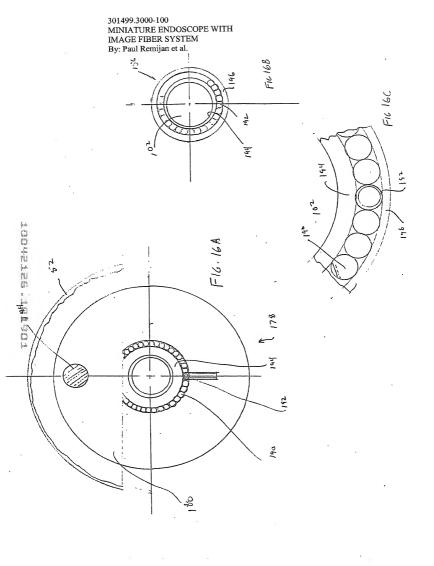

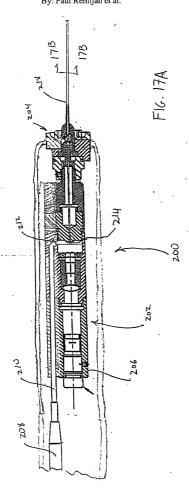

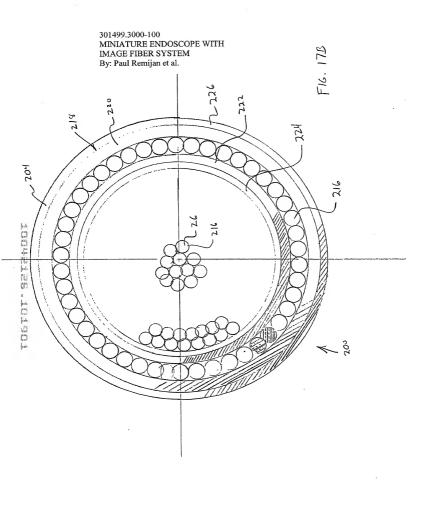

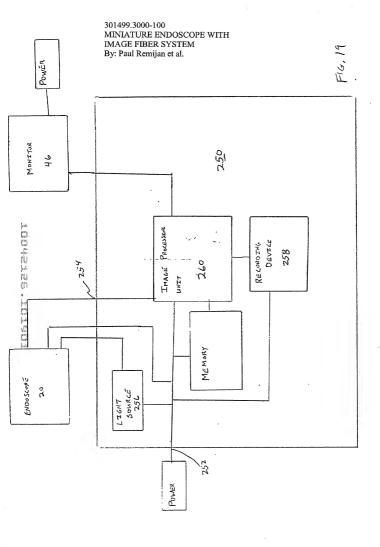

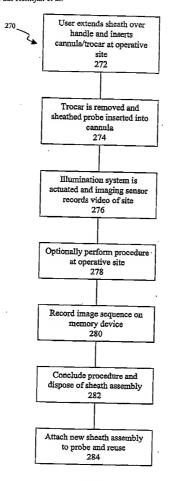


FIG. 20